



Microscope Systems for ICSI



Superior optical performance and precision for ICSI



Nikon microscopes have played a significant role from the early days of Intracytoplasmic Sperm Injection (ICSI) and continue to contribute to the advancement of this field through superior optical performance and precision.

This brochure introduces various ICSI products, including the latest inverted microscopes, manipulators and ThermoPlates necessary for ICSI, and upright and stereo microscopes used for ICSI-related work.



ECLIPSE Ti2 inverted microscope

The Ti2 provides an ultra-stable platform for carrying out precision manipulation procedures such as ICSI. The intermediate magnification switching function (1.5X) allows easy switching of observation magnifications between 200X and 300X without changing objectives. The stage can accommodate handles of various lengths on either the left or the right side. Combined with a variable inclination eyepiece tube, the Ti2 provides an ergonomic interface for precision manipulation. Both halogen and cell-friendly LED light sources are available for diascopic illumination. A motorized microscope model is also available.



ECLIPSE Ts2R inverted microscope

The Ts2R is smaller than the Ti2, while featuring the same stages, stage handles and eyepiece tubes. The compact design of the Ts2R enables it to fit easily inside clean benches or laminar flow hoods.

The Ts2R features an LED light source for diascopic illumination and the Ts2R-FL includes up to four additional fluorescent LED light sources. Users can quickly switch between diascopic and fluorescent observation by using buttons on the front panel. The Ts2R and Ts2R-FL can be configured for a variety of contrasting methods including Emboss Contrast, NAMC, and spindle observation.



SMZ18/SMZ1270/SMZ800N stereo microscopes

Zoom ratio is 18:1 (zoom range: 0.75X - 13.5X) with SMZ18, 12.7:1 (0.63X - 8X) with SMZ1270 and 8:1 (1X - 8X) with SMZ800N. The Oblique Coherent Contrast (OCC) option enables high-contrast observation of oocytes and embryos.



SMZ18

ECLIPSE Ci/ECLIPSE E200 upright microscopes

The Ci series offers three different models, all of which are compatible with phase contrast observation. The Ci-E and Ci-L feature an LED light source for diascope illumination which transmits minimal heat and is therefore ideal for sperm observation. The Ci-S is equipped with a halogen light source. The compact ECLIPSE E200 is available in both halogen and LED models.



ECLIPSE Ci-L



Accessories for Inverted Microscope



Nikon Advanced Modulation Contrast (NAMC) observation Ti2 Ts2R

The Nikon Advanced Modulation Contrast (NAMC) technique enables high-contrast observation of colorless and transparent samples through plasticware. NAMC produces a pseudo-relief shading effect, ideal for ICSI. The direction of shading can be adjusted through 360 degrees by turning the modulator in an NAMC objective. CFI S Plan Fluor ELWD NAMC objectives are equipped with a modulator ring clamping mechanism to prevent accidental rotation of the modulator ring while rotating the correction collar.



A sperm cell can be clearly observed in the injection pipette
 Images courtesy of: Derek Keating, B.A. and Gianpiero D. Palermo, MD, PhD., Andrology and Assisted Fertilization: Weill Cornell Medicine Ronald O. Perelman and Claudia Cohen Center for Reproductive Medicine.



CFI S Plan Fluor ELWD NAMC 20XC (left),
 CFI S Plan Fluor ELWD NAMC 40XC with clamp mechanism (right)


CFI Achromat NAMC 10XF (left),
 CFI Achromat LWD NAMC 20XF (middle),
 CFI Achromat LWD NAMC 40XC (right)

Spindle observation Ts2R

This polarized light technique enables finely detailed observation of spindle bodies for oocyte assessment and the elimination of spindle damage during sperm injection.

Switching between spindle observation and NAMC or Emboss Contrast is fast and easy as spindle observation only requires two optical modules, one mounted in the condenser turret and an analyzer inserted under the nosepiece.

The following five objectives are compatible with spindle observation: CFI Achromat LWD 40XC, CFI S Plan Fluor ELWD 20XC, CFI S Plan Fluor ELWD 40XC, CFI S Plan Fluor ELWD NAMC 20XC and CFI S Plan Fluor ELWD NAMC 40XC.

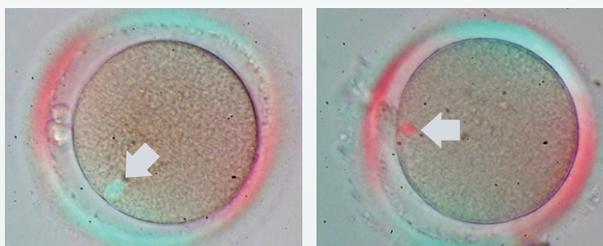

Spindle bodies (indicated by arrows) observed in different colors depending on their orientation. The color can be changed from blue to red by rotating the condenser module 90 degrees.



TS2R-C-SO Spindle Observation System



Emboss Contrast observation

Ts2R

The Emboss Contrast technique provides pseudo-relief contrast of samples on plasticware, similar to NAMC, but with less glare. Emboss Contrast is compatible with standard objectives and therefore easily combined with epi-fluorescence applications.



Image courtesy of Hideaki Watanabe, Ph.D. and Hisataka Hasegawa, Ph.D.



CFI Plan Fluor 10X, CFI S Plan Fluor ELWD 20XC,
CFI S Plan Fluor ELWD 40XC,
CFI S Plan Fluor ELWD 60XC



Stage

Ti2 Ts2R

Durable manual stages with smooth motion. Available with left or right handle positions and different handle lengths ("short" and "medium" for Ts2R and Ti2, and an additional "long" option for the Ti2).



Camera port for image projection and photo-documentation

Ts2R

The Ts2R's optional camera port is compatible with C-mount cameras (in combination with camera adapters). Three types of camera ports with different light split ratios are available for image sharing between the binocular tube and camera.

The TS2R-P-CHL Camera Port 50L is specifically designed for ICSI to ensure easy access to the stage.



Ts2R-FL configured with TS2R-P-CHL Camera Port 50L

NTX Micromanipulator set


Ti2

The NTX is a dedicated micromanipulator set for the Ti2 inverted microscope that allows effortless setup and easy adjustment of the pipette holder. Micromanipulator systems produced by a collaboration between Nikon and Narishige have earned high praise worldwide since their development.

*In the U.S.A. and Europe, use NTXVM for clinical use.

Newly designed dedicated adapter

The junction positions of the microscope's support section and the supporting parts of the motor-driven manipulator are set depending on each pipette's angle, and the angle of the pipette holder can be easily adjusted.

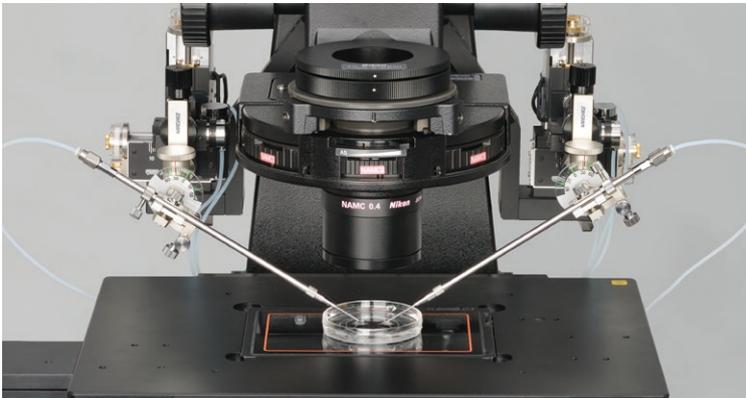

With pipette angle set to 35 degrees (high)



With pipette angle set to 20 degrees (low)

Improved stability

The set location of the pipette holder is positioned on the central shaft of the universal joint. It improves the stability of the pipette holder in combination with the novel mechanism.

The enlarged angle indicator and newly added angle index on the universal joint improve the readability of the pipette angle display.

In addition, pipettes can be manually moved up and down using the dial with an arrow displayed.



Improved operability

Operability is improved with reduced rebound risk and enhanced responsiveness.



Movement range

Knob operation	10 mm
Full knob rotation	250 μm
Minimum graduation	2 μm
Joystick operation	Max. 2 mm
Motorized operation	22 mm



Configuration with inverted microscope Ti2-U



MTK-1 Micromanipulator set


Ti2 Ts2R

The MTK-1 features smooth and accurate response from the joystick, improved rigidity of the manipulator and increased stability of the pipette position. It is a new type of micromanipulator for ICSI, with various features including instant change of pipette position and easy adjustment of pipette angle. It allows anyone to perform easy and secure pipette setting.

*In the U.S.A. and Europe, use MTK-1VM for clinical use.



- The pipette tip stays in the same position in the field of view, even when the pipette angle is changed.

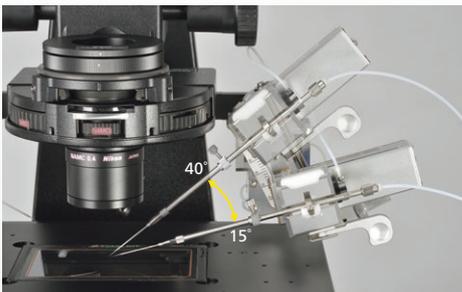


- Simple switching of the pipette setting between HOME and WORKING positions using a lever enables the fast and secure exchange of pipettes and dishes, preventing the breaking of pipettes.



WORKING position



HOME position

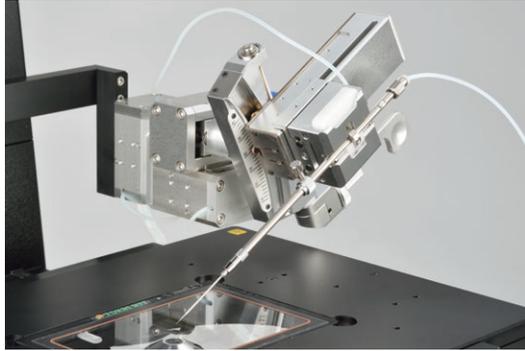

- Improved rigidity of the manipulator body for stable installation. It allows easy mounting on a microscope, and position adjustment.



- Oil hydraulic manipulator provides smooth and accurate response.

Movement range	Knob operation	10 mm (X, Y, Z and T axes)
	Full knob rotation	250 μm (X, Y and Z axes), 1,000 μm (T axis)
	Lever movement	50 mm (T axis)
Inclination angle of T axis		15 - 40°



Configuration with inverted microscope Ti2-U

Configuration with inverted microscope Ts2R-FL

Micromanipulator-dedicated microinjector

Pneumatic Microinjector IM-11-2

The IM-11-2 allows suction and injection of a microsample with precision and operability comparable to oil hydraulic injectors. It is suitable for both injecting and holding during ICSI. Air bubbles do not enter the micropipette when the pneumatic microinjector is fitted.

- Movement range: 40mm
- * In the U.S.A. and Europe, use IM-11-2VM for clinical use.



Oil-type Microinjector IM-9B

The IM-9B is suitable for injection and provides smoother and more stable maneuverability by employing a mechanism that minimizes backlash. Also, its 53mm working distance, large-volume syringe and just-the-right-size control knob with graduated scales all contribute to easy control of the injection.

- Movement range: 53mm (Full rotation of knob: 500 μ m)
- Control value: approx. 10 μ l with full rotation of knob (Glass type syringe: 1,060 μ l)
- * In the U.S.A. and Europe, use IM-9BVM for clinical use



Pipette Holder Clamper HIK-5N

The HIK-5N is used to keep the pipette holder in the desired position, thereby simplifying pipette exchange. The magnetic clamper can be attached to a bench or iron plate.



Micropipette Puller PC-100

The PC-100 is used to pull the glass capillary vertically, utilizing the gravitational force of its own weight. It has two modes: a single pull, pulling capillary at one stretch, and a double pull in which the setting is changed in mid-process.



Microforge MF-900

The MF-900 is designed to produce injection and holding pipettes. In addition to the temperature and illumination, the position of the heating element can be adjusted.



Pipette Grinder EG-401

The grinder with minimized irregular movements of the grinding plane and the microscope are combined. Precise grinding while confirming needle contact with grinding plane is facilitated.



Glass Capillaries G-100, G-1, GD-1/1.2/1.5

G-100 is a thin-walled glass capillary ideal for ICSI, while G-1 is for general purpose. The GD series is commonly known as double tubing. These glass capillaries contain an internal glass fiber (approx. 100 μm). The glass capillaries have been prewashed in an ultrasonic washing machine.



ThermoPlate® TPI series

TPI-TCSX for inverted microscope



Automatic thermocontrol system with a glass heating plate keeps the specimen at a set temperature. Temperature is adjustable from room temperature to 60°C in 0.1°C increments.

TPIE-SP/SPE



The TPIE-SP/SPE allows thermal control of standby samples beside a microscope. A large SP type and small SPE type are available.

TPIID-SMZ25DX for stereo microscope



The TPIID-SMZ25DX enables thermal control of standby samples as well as samples under observation. This is useful when dealing with multiple samples.

TPI-UNIX for stereo microscope



The TPI-UNIX can be used for all stereo microscope stands. The entire area of the glass heater is heated to control the temperature of multiple dishes.

Diascopic Illumination Stands with built-in OCC illuminator

Nikon's unique OCC oblique contrast technique applies coherent light to samples in a diagonal direction, by partially shading the optical path. This method provides relief-like contrast to colorless and transparent sample structures such as oocytes.


Two types of stand are available: the P-DSF32 Fiber Diascopic Illumination Stand that allows high-contrast illumination, and the compact, slim-type P-DSL32 LED Diascopic Illumination Stand that generates minimal heat.




Contrast can be optimized for a sample using the OCC adjustment knob on the P-DSF32 Fiber Diascopic Illumination Stand.



The slide lever with scales on the P-DSL32 LED Diascopic Illumination Stand allows the desired levels of OCC illumination to be saved and reproduced.

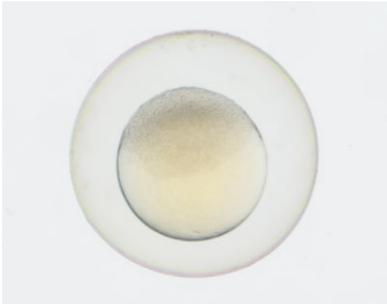

Normal diascopic illumination

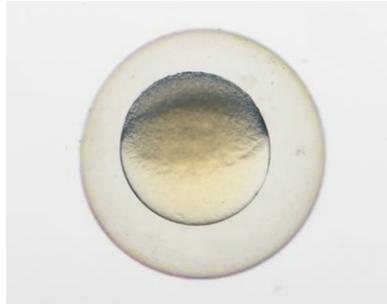

OCC illumination (with LED diascopic illumination stand)

Sample: Zebrafish embryo (using SHR Plan Apo 1X at zoom magnification of 5X with SMZ18)
Image courtesy of: Dr. Junichi Nakai, Ph.D. Saitama University Brain Science Institute



SMZ18 configured with P-DSF32 DIA Stand



SMZ1270 configured with P-DSF32 DIA Stand



SMZ800N configured with P-DSL32 DIA Stand

* Microscope cameras can be mounted via P-IBSS2 beam splitter S2



Accessories for Upright Microscope

Phase contrast accessories for ECLIPSE Ci

As it enhances the contrast of samples, phase contrast observation is effective for the measurement of sperm count or sperm motility using the Computer-Assisted Sperm Analysis (CASA) system. Dedicated objectives and a dedicated condenser are required for phase contrast technique.



- ① CFI Plan Fluor DLL 10X, 20X, 40X, 100X Oil phase contrast objectives
- ② C-CT Centering Telescope
- ③ C-PH Phase Contrast Turret Condenser
- ④ CI-F-CH Filter Cassette Holder



Ci-L configured with phase contrast accessories

Phase Contrast Objectives for Sperm Observation

CFI Plan Fluor BM 40X and CFI BM 10X objectives provide bright, negative phase contrast images, ideal for sperm observation. The parts of samples that have large phase differences are visualized as bright objects against a dark background, similar to darkfield microscopy. It is particularly useful for observing terminal filaments of sperm flagella.



Sperm of echinus
Images courtesy of: Dr. Sumio Ishijima,
Tokyo Institute of Technology



CFI Plan Fluor BM 40X

Phase contrast accessories for ECLIPSE E200




- ① GIF Filter, ② Centering Telescope, ③ E2 Phase Contrast Condenser,
- ④ Phase Contrast Slider 10X-40X, ⑤ Phase Contrast Slider 100X




CFI Achromat DL 10X, 20X, 40X, 100X Oil phase contrast objectives



ECLIPSE E200-F
(model with field diaphragm)

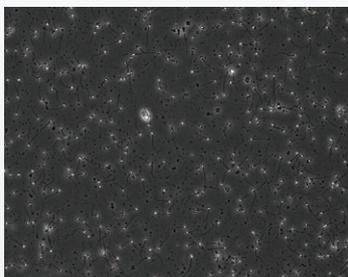

Phase contrast image of sperm

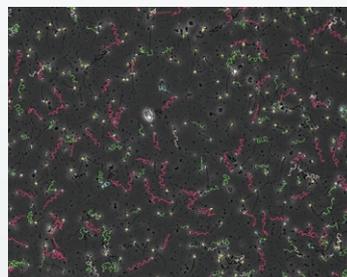

Sperm tracing image, color-coded according to sperm velocity.

Objective: CFI Achromat DL 10X
Images courtesy of: DITECT corporation
(Sperm Motility Analysis System: SMAS)

Microscope Camera DS-Fi3

The DS-Fi3 is a high-definition color camera equipped with a 5.9 megapixel CMOS image sensor. With its high-speed data readout and superior color reproduction, the DS-Fi3 is an ideal camera for a variety of observation techniques.

- Max recordable pixels: 2880 × 2048



Microscope Camera Control Unit DS-L4

The DS-L4 is a compact, easy-to-operate, tablet-type camera control unit with a large, 10.1 inch touch panel display, allowing easy sharing of live images and photo-documentation. The DS-L4 has a large number of built-in functions for measurement and annotations, and has built-in security for network connectivity.



Photographed at, and with the cooperation of:

Reproduction Clinic Tokyo
Tokiwadai Ladies Clinic

Micromanipulators and related equipment are manufactured by:



NARISHIGE CO., LTD.

27-9, Minamikarasuyama 4-chome, Setagaya-ku, Tokyo 157-0062, Japan
phone: +81-3-3308-8383 fax: +81-3-3308-8700
e-mail: sales@narishige.co.jp
<http://narishige-group.com>

ThermoPlate® is manufactured by:



Tokai Hit CO., LTD.

306-1 Gendoji-Cho, Fujinomiya-shi, Shizuoka-ken 418-0074, Japan
phone: +81-544-24-6699 fax: +81-544-24-6641
e-mail: solution@tokaihit.com
<http://www.tokaihit.com>

Specifications and equipment are subject to change without any notice or obligation on the part of the manufacturer. August 2018
©2018 NIKON CORPORATION

 WARNING	TO ENSURE CORRECT USAGE, READ THE CORRESPONDING MANUALS CAREFULLY BEFORE USING YOUR EQUIPMENT.
---	--

N.B. Export of the products* in this brochure is controlled under the Japanese Foreign Exchange and Foreign Trade Law. Appropriate export procedure shall be required in case of export from Japan. *Products: Hardware and its technical information (including software)



NIKON CORPORATION

Shinagawa Intercity Tower C, 2-15-3, Konan, Minato-ku, Tokyo 108-6290, Japan
phone: +81-3-6433-3705 fax: +81-3-6433-3785
<http://www.nikon.com/products/microscope-solutions/>

ISO 14001 Certified for NIKON CORPORATION
--

NIKON INSTRUMENTS INC.

1300 Walt Whitman Road, Melville, N.Y. 11747-3064, U.S.A.
phone: +1-631-547-8500; +1-800-52-NIKON (within the U.S.A. only)
fax: +1-631-547-0306
<http://www.nikoninstruments.com/>

NIKON INSTRUMENTS EUROPE B.V.

Tripolis 100, Burgerveeshuispad 101, 1076 ER Amsterdam, The Netherlands
phone: +31-20-7099-000 fax: +31-20-7099-298
<http://www.nikoninstruments.eu/>

NIKON INSTRUMENTS (SHANGHAI) CO., LTD.

CHINA phone: +86-21-6841-2050 fax: +86-21-6841-2060
(Beijing branch) phone: +86-10-5831-2028 fax: +86-10-5831-2026
(Guangzhou branch) phone: +86-20-3882-0550 fax: +86-20-3882-0580

NIKON CANADA INC.

CANADA phone: +1-905-602-9676 fax: +1-905-602-9953

NIKON FRANCE S.A.S.

FRANCE phone: +33-1-4516-45-16 fax: +33-1-4516-45-55

NIKON GMBH

GERMANY phone: +49-211-941-42-20 fax: +49-211-941-43-22

NIKON INSTRUMENTS S.p.A.

ITALY phone: +39-55-300-96-01 fax: +39-55-30-09-93

NIKON GMBH SWITZERLAND

SWITZERLAND phone: +41-43-277-28-67 fax: +41-43-277-28-61

NIKON UK LTD.

UNITED KINGDOM phone: +44-208-247-1717 fax: +44-208-541-4584

NIKON CEE GMBH

AUSTRIA phone: +43-1-972-6111 fax: +43-1-972-611-140

NIKON SINGAPORE PTE LTD

SINGAPORE phone: +65-6559-3651 fax: +65-6559-3668

NIKON INSTRUMENTS KOREA CO., LTD.

KOREA phone: +82-2-2186-8400 fax: +82-2-555-4415